




Instruction Manual

Model: Digital TENS Unit

Item # : 21005

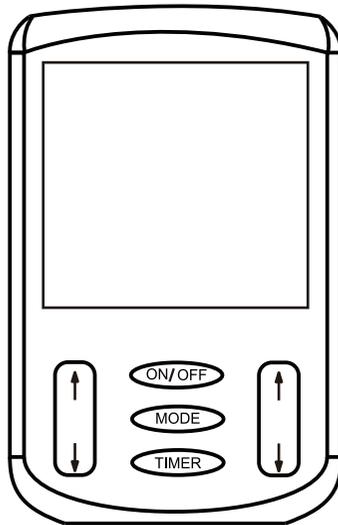

Please keep this instruction manual safe for future use.

TABLE OF CONTENTS

Introduction to TENS.....	02
Indications / Contraindications / Warnings.....	03
Contents	06
Description of device and functional buttons.....	07
Explanation of treatment modes.....	08
Explanation of parameter controls.....	08
Preparation for use.....	09
Electrodes and electrodes placement.....	10
Programming your device as a TENS.....	11
Programming the timer.....	12
Using the device.....	12
Ending your treatment session.....	12
Special features.....	13
Caring for your device.....	13
Changing the battery.....	14
Troubleshooting.....	15
Technical Specifications.....	15

Chapter 1: INTRODUCTION TO TENS

(1) GENERAL DESCRIPTION

The device is a battery operated pulse generator that sends electrical impulses through electrodes to the body to reach nerves causing pain. Electrical impulses can be adjusted by changing the pulse width and rate. The strength is individually adjusted using the 2 channels. A slide button (button lock function) protects the device from accidental changes while in use.

(2) EXPLANATION OF PAIN

Pain is the body's natural warning mechanism and is intended to prevent additional injury. Pain is important, as without it, vital parts of our body might be injured or damaged without our knowledge. While ointments, drugs or even surgery can be used to treat chronic pain, these are all utilized with varying degrees of success, as each individual patient and condition is different. TENS offers a unique alternative method of pain relief with no potentially harmful side effects.

(3) WHAT IS TENS

TENS, Transcutaneous Electrical Nerve Stimulator, is a battery powered electrical unit which uses electrodes placed onto the skin over a painful area to deliver electrical impulses to the nerve fibers which lie underneath the skin surface. It provides pain relief by blocking pain signals to the brain via the spinal cord and peripheral nervous system. TENS also stimulates production of endorphins, the body's own "painkillers".

(4) COMMON APPLICATIONS FOR TENS

Although dependent on your specific pain problem, TENS devices have been used successfully to treat many conditions, including:

CHRONIC PAIN

Cervical (Neck) – Amputation – Phantom Limb – Headache – Lower Back – Lumbago – Leg Pain – Arthritis

ACUTE PAIN

Post Operative – Muscle and Joint – Tendonitis – Fractures – Tennis Elbow

Chapter 2: INDICATIONS / CONTRAINDICATIONS / WARNINGS

CAUTION: Federal law (USA) requires this device to be sold only by or on the order of a physician (or licensed practitioner).

Read the operation manual in its entirety before using the device.

INDICATIONS:

This device may be used, with a physician/clinician's prescription, for the symptomatic relief and management of chronic (long term) pain and for the treatment of post-operative and post-traumatic pain.

CONTRAINDICATIONS

- **Heart Disease** – Use caution prior to using this device on patients suspected of having heart disease.
- **Cardiac pacemakers** – Do not use this device if you have a demand-type cardiac pacemaker or any implanted defibrillator.
- **Trans cerebral stimulation** – Do not apply electrical stimulation trans cerebrally (through the head).
- **Epilepsy** – Use caution for patients with suspected or diagnosed epilepsy when using this device.
- **Carotid sinus** – Do not apply electrical stimulation to carotid sinus region of the neck.
- **Unknown etiology** – Do not use this device if pain symptoms are undiagnosed. Use only after the origin / caused of pain has been determined by your doctor.
- **Hemorrhages** – Use caution when there is a tendency to hemorrhage, such as following acute trauma or fracture.
- **Post-surgical use** – Use caution following recent surgical procedures when muscle contraction may disrupt the healing process.
- **Uterus** – Do not use electrical stimulation during menstruation.
- **Sensory loss** – Do not use electrical stimulation where sensory nerve damage is present by a loss of normal skin sensation.
- **Skin irritation** – If patient experiences skin irritation due to electrical stimulation, stop using the device and consult the clinician. Irritation may be reduced by an alternative conductive medium or an alternative electrode placement. Isolated cases of skin irritation may occur at the site of electrode placement following long term application.
- **Adverse reactions** – In addition to skin irritation, inflammation and burns beneath the electrodes are potential adverse reactions. Follow directions carefully.

WARNINGS


- **Pregnancy** – The safety of using electrical stimulation during pregnancy or birth has not been established.
- **Central origin pain** – This device is not effective for pain of central origin (including headaches).
- **Prescription** – Use electrical stimulation only in the prescribed manner and for the prescribed reason.
- **Symptomatic treatment** – This device is a symptomatic treatment and, as such, suppresses the sensation of pain which would otherwise serve as a protective or warning mechanism of your body.
- **Keep out of reach of children** – Do not store or use this device near children.
- **Electronic equipment** – Electronic monitoring equipment (such as ECG and EKG alarms) may not operate properly when electrical stimulation devices are in use.
- **Machinery operation** – Never operate potentially dangerous machinery such as power saws, automobiles, etc. while using this device.
- **Uncomfortable stimulation** – If the stimulation levels are uncomfortable or become uncomfortable, reduce the intensity (amplitude) to a comfortable level. Contact your physician / clinician if this does not resolve the problem or if the problem persists or re-occurs at your next prescribed treatments session.
- **Neck stimulation** – Do not place electrodes across the neck or mouth. Severe spasm of the laryngeal and pharyngeal muscles may occur. This may be strong enough to close off the airway or cause breathing difficulty.
- **Long-term effects** – The long-term effects of chronic use of electrical stimulation are unknown.
- **Damage from liquids** – Do not immerse the stimulator unit in water or other liquids.
- **High frequency surgical devices** – Simultaneous connection of a patient to a high frequency surgical device while using this device may result in burns at the site of the electrodes and possible damage to the stimulator. Discontinue use before surgery.
- **Microwave or radio frequency sources** – Operation in close proximity to shortwave or microwave therapy equipment may shut the stimulator off.
- **Flammable** – Do not use the device in an environment where flammable or explosive fumes may exist.
- **External use** – This device is for external use only
- **Lead connection** – Do not connect the lead wires to an alternating current (AC) power source or other equipment not

▲ Danger


The device does not have AAP/APG protection.

Extreme hazard is possible if used in the presence of explosives, flammable materials or flammable anesthetics. Caution should be used when applying the device to patients suspected of having heart conditions. Further clinical data is needed to show if there are adverse side effects on those with coronary disease.


Chapter 3: CONTENTS



Combo unit



4 Electrodes




Storage bag



2 wires



3 AAA batteries




Instruction Manual



Warranty card


Chapter 4: DESCRIPTION OF DEVICE AND FUNCTIONAL BUTTONS

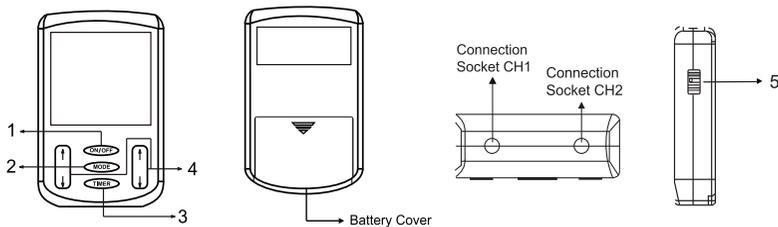

1. ON/OFF Button: Turns the power on and off.
2. MODE Button: Used to program the device.
3. TIMER Button: Used to program timer, 5 – 95 minutes or continuous (5 minute increments).
4. ↑ ↓ Buttons:
 - (i) Adjust MODE settings.
 - (ii) Adjust TIMER settings.
 - (iii) Increase / decrease the level of intensity for CH 1 and CH 2.
5. Sliding Switch: Lock / unlock buttons

The LCD Display:

1. Intensity level for Ch1 & Ch2 (30 levels)
2. System function (TENS)
3. Modes (3 different Modes)
4. Parameter setting (pulse rate / pulse width)
5. Timer (5-95 min. and continuous)
6. Symbol of button lock function
7. Low battery indicator



Chapter 5: EXPLANATION OF TREATMENT MODES

TENS Modes:

B: Burst mode consists of seven pulses at 100 Hz pulse rate. Burst occurs twice every second.

C: Constant mode keeps pulse rate and width at a constant level.

M: Modulation mode modulates between the control setting and 60% below control setting.

Chapter 6: EXPLANATION OF PARAMETER CONTROLS

Pulse Width:

Wider pulse duration settings will deliver stronger stimulation for any given intensity setting. The choice of which pulse duration to use is partially dependent upon the treatment mode selected.

Pulse Rate:

The pulse rate determines hertz or impulses per second.

Chapter 7: PREPARATION FOR USE

Insert batteries:

Your device operates with 3 AAA batteries. Please install batteries with polarities as indicated. Make sure the battery strip is placed below the batteries.

CAUTION: Never force a battery into the battery compartment. A battery that does not fit can damage the stimulator. This device requires 3 AAA batteries, never attempt to use any other battery type.

Preparing the Skin for a Therapy Session:

Proper preparation of the skin is essential to prolong electrode life and reduce the risk of skin irritation.


To prepare your skin at the electrode placement sites:

1. Determine the placement sites for the electrodes. Follow your clinician's instructions.
NOTE: Your clinician generally has you place the electrodes above and below (or surrounding) the area of pain or along the "pain path" of your arm or leg.
2. Wash the area with mild soap and water (do not use alcohol). Rinse and dry thoroughly.
3. Trim excess body hair from the area with scissors (do not shave).
4. Optionally, apply skin prep to the area to form a protective barrier on your skin.
5. When removing electrodes, always remove by pulling in the direction of hair growth. Do NOT pull on the wire.
6. It may be helpful to apply skin lotion on electrode placement area when not wearing electrodes.

Connecting the electrodes to the device:

Hold the insulated portion of the electrode connector and push the plug end of the lead wire into the electrode connector. Repeat for all 4 electrodes. After connecting each electrode, plug the other end of the lead wire into the TENS device.

Caution: The device should be OFF before connecting the lead wire to the TENS device.

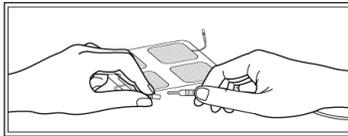

Note: Use care when you plug and unplug the wires. Pulling on the lead wire instead of its insulated connector may cause wire breakage.

Caution: Never insert the plug of the lead wire into an AC power supply or other equipment not specified as safe for the lead wires.

Chapter 8: ELECTRODES AND ELECTRODE PLACEMENT

General electrode information:

Electrodes should be routinely replaced when they start to lose their adhesive nature. If you are unsure of your electrode adhesive properties, order replacement electrodes. Replacement electrodes should be re-ordered through your local dealer or call Zewa customer service. Follow application procedures outlined on electrode packaging to maintain optimal stimulation and to prevent skin irritation.

Electrode Placement:

The placement of electrodes can be one of the most important parameters in achieving success with TENS therapy. Of utmost importance is the willingness of the clinician to try the various styles of electrode placement to find which method best fits the needs of the individual patient. Every patient responds to electrical stimulation differently and their needs may vary from the conventional setting suggested here. If the initial results are not positive, feel free to experiment. Once an acceptable placement has been achieved, mark down the electrodes sites and the settings, so that the patient can easily continue treatment at home.

Contiguous Electrode Placement:

This is the most common placement technique. It involves pacing the electrodes alongside the area of localized pain sites, in such a way as to direct the flow of current through or around the area of pain. In a single channel application, this would involve placing each electrode on either side of the pain site if the pain is localized on the limb and deep within the tissue. Electrode placement on the posterior and anterior aspects of the affected limb will allow the current to flow completely through the limb and thus through the endogenous pain site. With a 2 channel application, the clinician may either direct the current flow to cross through the pain site or in what is called the "bracket" method allowing the current flow on either side of the painful area, generally through the nerve branches that feed into the pain site.

Note: Electrodes should be placed between 0.5" – 2" apart from each other.

Caution: The device should be in the OFF position before placing the electrodes on your skin.

Chapter 9: PROGRAMMING YOUR DEVICE

1. Turn the device ON

- Press "ON/OFF" button to turn the unit ON.
- The most recently selected treatment status is displayed.

2. Turn the device OFF

- The device turns off automatically after the therapy session time has elapsed.
- The device will turn off after 60 seconds if no button is pushed.
- To turn the unit off manually, press "ON/OFF" button for 3 seconds.

Note: To prevent unpleasant electric shocks, never move the lead wires or electrodes while the device is still turned on.

3. Mode Selection

The device features 3 different Modes: Constant (C), Burst (B), Modulated Width (M).

- To change the Mode, press the "MODE" button. The device will display your settings. Press "MODE" again and your last selected Mode will start flashing.
- To make changes, press the "UP" or "DOWN" button.
- Once you have selected your Mode, press the "MODE" button again and the pulse rate starts flashing. Continue with step 4.

4. Parameter Setting (pulse rate and width)

To adjust the pulse width and pulse rate settings, follow these steps:

- To adjust the pulse rate (Hz), push the "UP" or "DOWN" button (1 – 150Hz).
- Press the "MODE" button and the pulse width starts flashing (uS). Press the "UP" or "DOWN" button to change the pulse width (30 – 300uS).
- Once you are done changing the pulse rate and pulse width, press the "MODE" button and the display stops flashing indicating your programming is finished. The display will show your final programming.

Note 1:

When the device is in use and the "MODE" button is pushed 1 time, it will show the current programming. To make changes, press the "MODE" button again, all intensity levels will turn to "0" and the mode function will start flashing. Please follow above steps to make changes.

Note 2:

If no button is pushed for 10 seconds while in programming mode, the device will stop flashing. To return into programming mode follow steps above by pressing the "MODE" button.

Note 3:

If the device is in programming mode (intensity bars are at "0"), the device will automatically turn OFF after 60 seconds if no button is pushed.

Chapter 11: PROGRAMMING THE TIMER

To program the timer, follow these steps:

- Press the "TIMER" button and the timer will start flashing.
- Press the "UP" or "DOWN" button to adjust the time.
- Press the "TIMER" button to save the changes or wait 10 seconds until the timer stops flashing.

Chapter 12: USING THE DEVICE

1. Connect the electrodes to the TENS control unit.
2. Place electrodes on your skin.
3. Turn the Device ON by pressing the "ON/OFF" button.
4. Using the intensity control buttons, change the intensity for each channel (Note: intensity will increase at a lower rate for the first 10 intensity levels and increase at a faster rate from level 11 to 30).
5. The device will turn off automatically if the timer was set (count down minutes are shown on the display). If it was set to C (continuous) the device has to be turned OFF manually.
6. To turn the device OFF manually, press the "ON/OFF" button for 3 seconds.

Chapter 13: ENDING YOUR TREATMENT SESSION

After the device shuts off, use the following steps as a quick reference for ending your session:

- Disconnect the lead wire(s) from the control unit.
- Remove electrodes from skin and place them back on the transparent liner. When removing electrodes, always pull in the direction of hair growth. **DO NOT REMOVE ELECTRODES WHILE THEY ARE CONNECTED TO THE UNIT TO AVOID ANY ELECTRIC DISCHARGE.** Do NOT pull on the wires, but peel off on the corner of the electrode.
- Disconnect the lead wire(s) from the electrodes.
- Store the components in the storage bag.

Chapter 14: SPECIAL FEATURES

Button Lock Function:

Slide the sliding switch to lock or unlock. The lock feature will lock all buttons so that no accidental changes can be made during a treatment.

Automatic Shutoff

- The device turns off automatically when not in use and no button is pressed for 60 seconds.
- The device will turn off automatically when the timer reaches “0” minutes.

Intensity Level Reset

1. For your safety and comfort, the intensity level will reset to 0 each time the device is turned off, including after a therapy session.
2. For your safety and comfort, the intensity level will reset to 0 in case the device is changed into programming mode (pressing the “MODE” button 2 times).

Low Battery Indicator

The low battery indicator is displayed whenever the battery is low. The battery needs to be changed.

Programming Recall

The last treatment and timer setting is automatically saved and will appear on the display when the device is turned on for the next treatment.

Chapter 15: CARING FOR YOUR DEVICE

The device may be cleaned by gently wiping it with a damp cloth moistened with mild soap and water. **Never immerse the device in water or other liquids.**

Wipe lead wires with a damp cloth as described above if they become soiled.

To properly store the device for an extended period of time, remove the battery from the device. Put the device and accessories in the storage bag and store in a cool dry location.

Chapter 16: CHANGING THE BATTERY

- When the low battery symbol is displayed, the battery is too weak to power the device and it is time to change it. At this point, the device will shut off until a fresh battery is inserted. If you decide to install a new battery before the device has shut itself off, be sure to turn the power off before you undertake to change the battery.
- To change the battery, open the battery compartment as you did when you first installed it. Pull out the old batteries and insert new ones according to directions.

CAUTIONS:

- 1. Do not connect the stimulator to any electrical outlet.**
- 2. Remove batteries from the device during storage to prevent battery leakage. Failure to do so may damage the device.**
- 3. Replace battery if device was immersed in water or liquid.**
- 4. Never recharge alkaline batteries. An explosion may result.**
- 5. Dispose of all batteries according to current federal, state, and local regulations.**

Chapter 17: TROUBLESHOOTING

If your device does not function properly:

Problem	Possible Cause	Solution
Stimulation is weak	<ol style="list-style-type: none"> 1. Low Batteries 2. Poor electrode contact 3. Worn electrodes 	<ol style="list-style-type: none"> 1. Change Batteries 1. Reapply electrodes, secure firmly 2. Replace electrodes
Stimulation stops	<ol style="list-style-type: none"> 1. Low Batteries 2. Poor electrode contact 3. Damaged or worn lead wires and/or electrodes 4. Therapy time complete 	<ol style="list-style-type: none"> 1. Change Batteries 2. Reapply electrodes, secure firmly 3. Replace lead wires and/or electrodes 4. Restart device
Stimulation weakens with minutes after start	Normal "adaptation" response	Increase intensity
Unintentional muscle contractions	Intensity too high	Decrease intensity
Stimulation uncomfortable	<ol style="list-style-type: none"> 1. Intensity too high 2. Improper electrode placement 3. Poor electrode contact 	<ol style="list-style-type: none"> 1. Decrease intensity 2. Reposition electrodes 3. Reapply electrodes, secure firmly
Stimulation ineffective	Improper electrode placement	Reposition electrodes

Note: If there is any other problem, please call Zewa customer service at 1-888-993-3592.

Chapter 18: TECHNICAL SPECIFICATIONS

Wave form	Asymmetrical Bi-Phasic square pulse
Channel	Dual, isolated between channels.
Modes	3 Modes
Pulse Intensity	Adjustable 0-100mA peak into 500 ohm load each channel
Pulse Rate	1-150Hz
Pulse Width	30-300uS
Timer	5 – 95 min. and continuous
Power source	3 x AAA Batteries (4.5V)

Model: Digital TENS Unit

Manufactured for Zewa, Inc.
12960 Commerce Lakes Drive # 29
Fort Myers, FL 33913
USA
www.zewa.com

Toll Free Customer Service:
1-888-993-3592

IM-25-003 RevA12